

# Application News

## No. A513

### Spectrophotometric Analysis

## Measuring Micro-Contaminants on Optical Parts: Measurement and Identification by AIM-9000 Infrared Microscope

Due to the miniaturization and increasingly sophisticated functionality of electrical and electronic devices, an increasing number of optical devices are being used today, such as ultra-small and high-performance semiconductor devices and sensors. However, in such miniaturized devices, micron-sized tiny contaminants can cause the devices to malfunction. Therefore, manufacturers need to determine what caused such contaminants to enter the devices, so their recurrence can be prevented.

Shimadzu AIM-9000 infrared microscope features optics that are designed especially for measuring microscopic areas, and allows users to obtain good spectra in short time even for micron-sized tiny contaminants. The following describes an example of using this system to measure micro-contaminants about 10  $\mu\text{m}$  in diameter on the surface of an optical part.

#### Micro-Contaminants on an Optical Part


Fig. 1 shows a microscope photograph of the contaminants on the surface of an optical part installed in an electronic device. The contaminants, which are between about 3 and 10  $\mu\text{m}$  in diameter, are lying scattered on a part surface.



**Fig. 1** Microscope Image of Micro-Contaminants (shown with a 10  $\mu\text{m}$  blue box)

#### Measurement

These contaminants were discovered on a shiny, flat, and smooth metal part surface. Therefore, a measurement using specular reflection spectroscopy is appropriate due to no necessity of sampling the part and the low risk of part damage or loss. An infrared spectrum measured from the contaminant using an infrared microscope by specular reflection spectroscopy and corresponding search results are shown in Fig. 2. Measurement conditions are indicated in Table 1. Even for tiny contaminants only about 10  $\mu\text{m}$  across, a spectrum with minimal noise can be obtained using a short measurement time of only about 20 seconds. Results from analyzing the data using the spectrum library included standard with the system determined that the contaminant is probably a lactate.

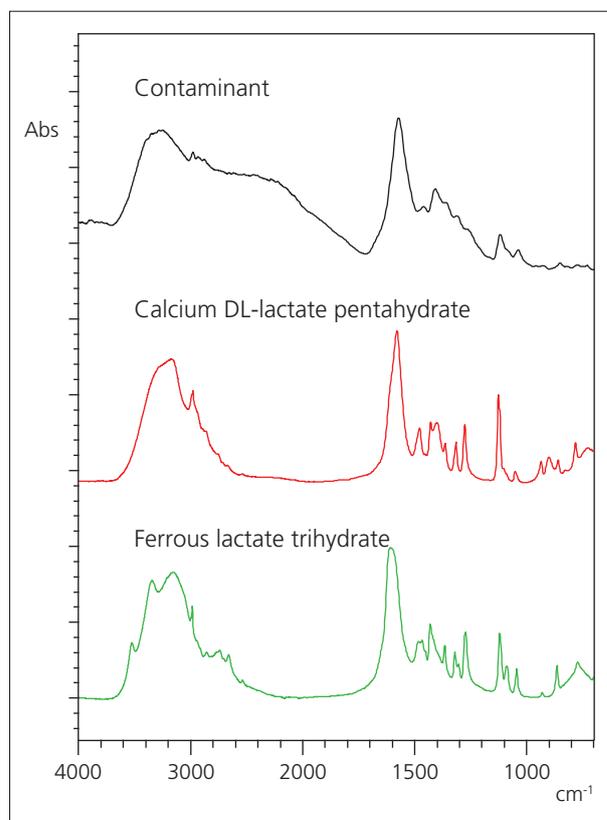


**Fig. 2** Infrared Spectrum and Search Results for the Contaminant

**Table 1** Measurement Conditions

Instrument	: IRTracer-100, AIM-9000
Resolution	: 8 $\text{cm}^{-1}$
Accumulation	: 40
Apodization	: Happ-Genzel
Detector	: MCT

### ■ AIM-9000 Infrared Microscope


Due to the optics that are designed specifically for measuring extremely small areas, the AIM-9000 infrared microscope achieves the highest signal-to-noise ratios (30,000:1) in its class. That means it can obtain excellent spectra very quickly, even from extremely small contaminants. As an example, results from measuring 10 µm polystyrene beads scattered on a BaF<sub>2</sub> window plate are shown. A microscope photograph of the polystyrene beads is shown in Fig. 3. A comparison of measurements obtained by transmission spectroscopy using both the AIM-9000 and the Shimadzu's previous model is shown in Fig. 4. Measurement conditions are listed in Table 2 and a photograph of the AIM-9000 system connected to an IRTracer-100 infrared spectrophotometer is shown in Fig. 5.

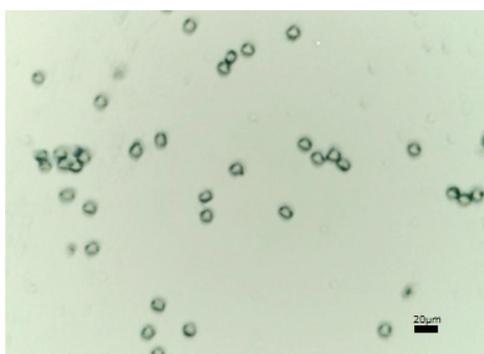

**Fig. 3 Microscope Image of Polystyrene Beads of 10 µm in Diameter**

**Table 2 Measurement Conditions**

Instrument	: IRTracer-100, AIM-9000, and previous model (AIM-8800)
Resolution	: 8 cm <sup>-1</sup>
Accumulation	: 40
Apodization	: Happ-Genzel
Detector	: MCT

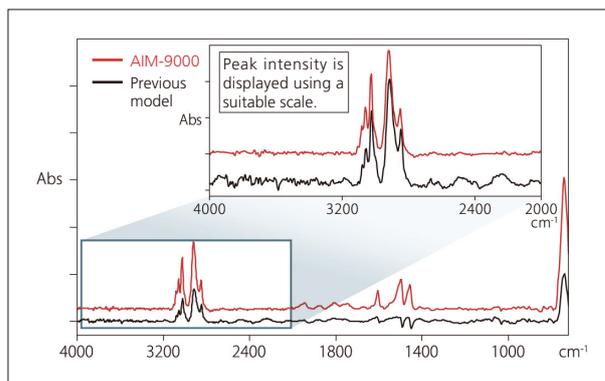

**Fig. 4 Infrared Spectra of Polystyrene Beads of 10 µm in Diameter (with Baseline Correction)**

These results show that the AIM-9000 detects the polystyrene absorption peaks more clearly and with higher intensity. The inset enlargement shows the results from displaying the spectra with peak intensity matched near 2,920 cm<sup>-1</sup>. It demonstrates how the AIM-9000 can provide superior spectra with less noise than the previous model.

### ■ Conclusion

This article describes measuring micro-contaminants about 10 µm in diameter on the surface of an optical part. The AIM-9000 infrared microscope is ideal for identifying contaminants and analyzing defects in extremely small areas.



**Fig. 5 AIM-9000 Infrared Microscope Connected to IRTracer-100 Fourier Transform Infrared Spectrophotometer**

First Edition: Nov. 2016



Shimadzu Corporation  
www.shimadzu.com/an/

**For Research Use Only. Not for use in diagnostic procedure.**

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Company names, product/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation or its affiliates, whether or not they are used with trademark symbol "TM" or "®". Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services. Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.